

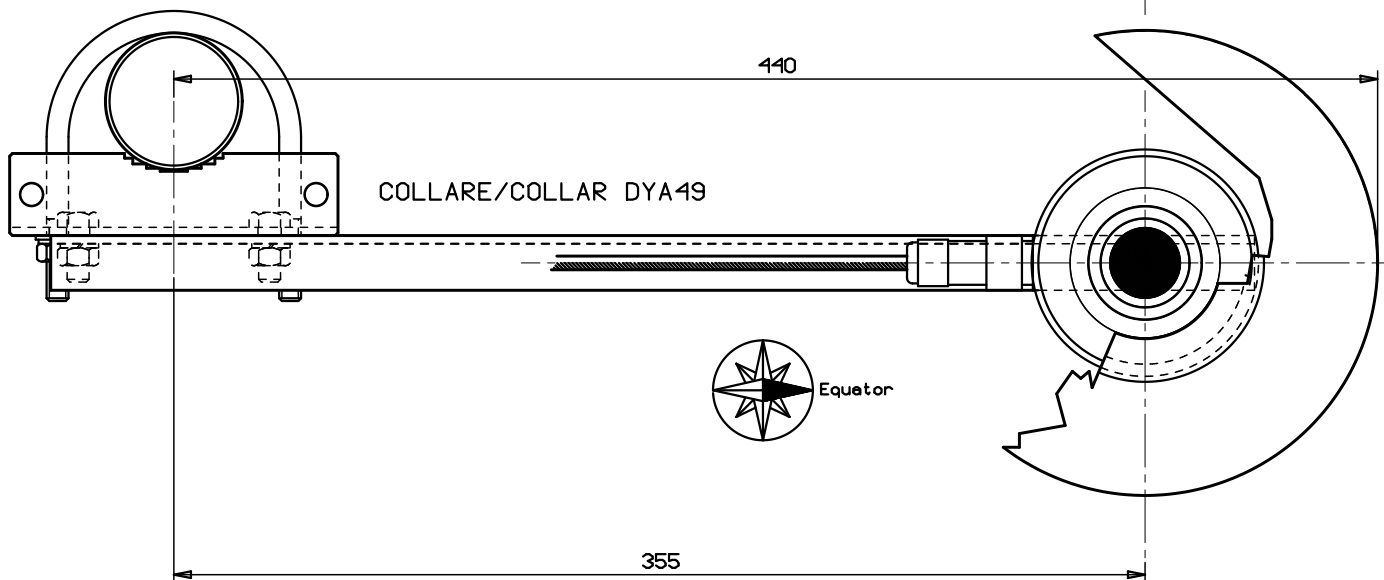


Cod: DPA252 : CAMPO/RANGE 285..3000nm;0..4000W/m²
SENSITIVITA'/SENSITIVITY 4..25μV/(W/m²)


Cod: DPA852 : ALIM./POWER SUPPLY 7..35V= CAMPO/RANGE 285..3000nm;0..4000W/m²
USCITA/OUTPUT 4..20mA

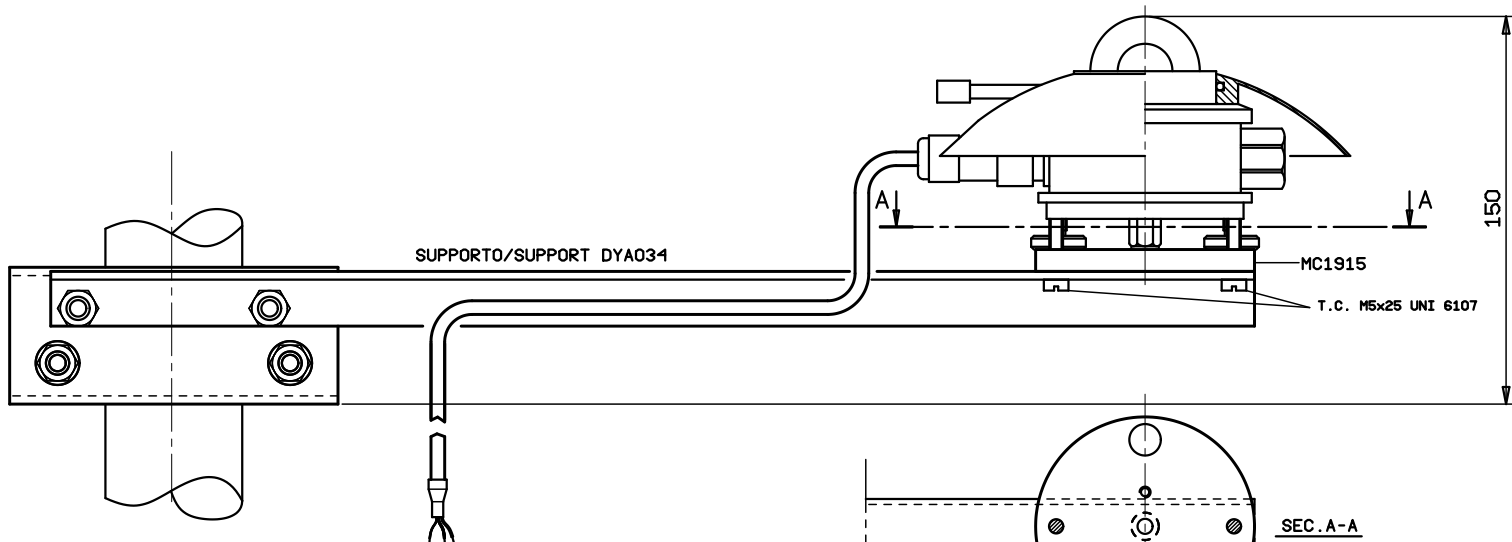

SCHEMA GENERICO DI CONNESSIONE
ELETTRICA A DATA LOGGER E/R/M-Log
GENERIC ELECTRICAL CONNECTION
TO E/R/M-Log DATA LOGGER
MORSETTIERA/TERMINAL BOARD
VEDI MANUALE UTENTE DATA LOGGER
SEE DATA LOGGER USER'S MANUAL

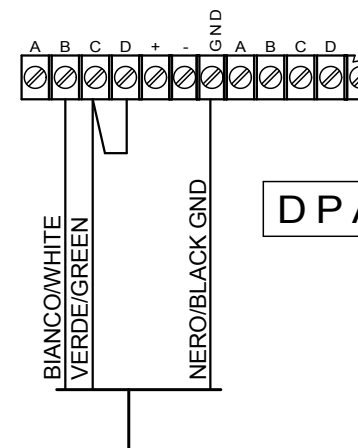

DPA252

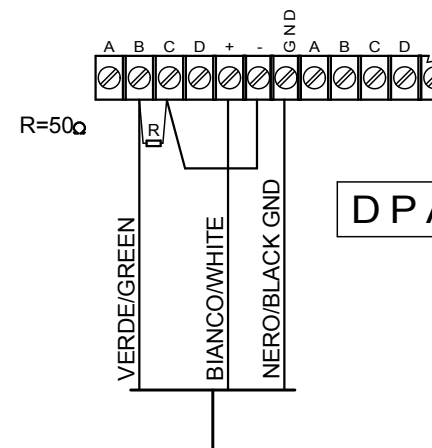

DPA852

a						Descrizione delle revisione	
Origine	15-09-14	A.A.	CGC	A.As.	A.As.	Materiale:	
Esp.di revisione	Date	(R)	(C)	(V)	(A)	Disegno:	
LSI LASTEM						Codice: DPA252 DPA852	DISACC6195
Descrizione: PIRANOMETRO STANDARD SECONDARIO (ISO 9060) PYRANOMETER SECONDARY STANDARD (ISO 9060)							